Instruction Sheet

Random Tandem Connection (Front-to-back)

Primary Section

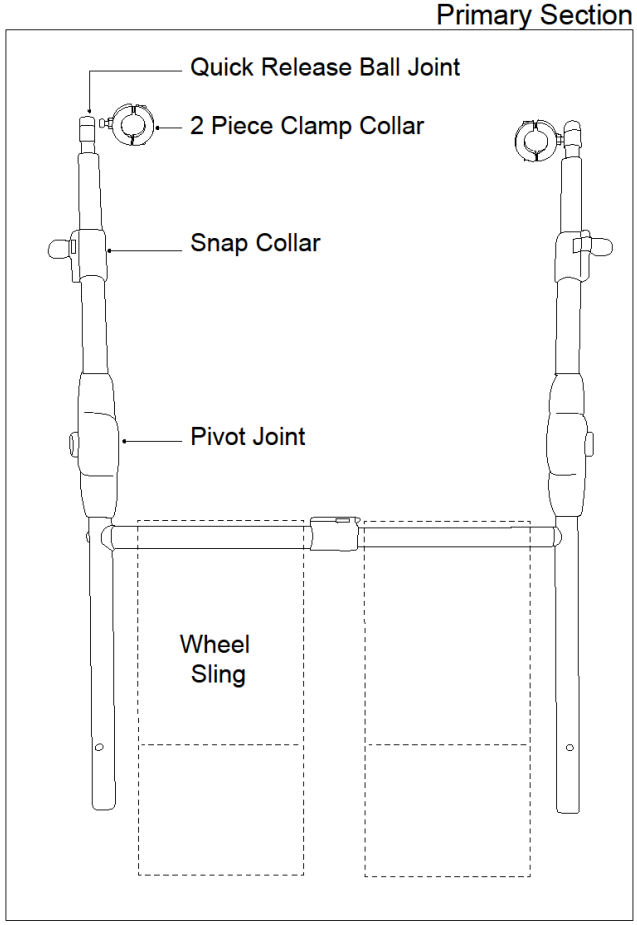

Wheeled Section

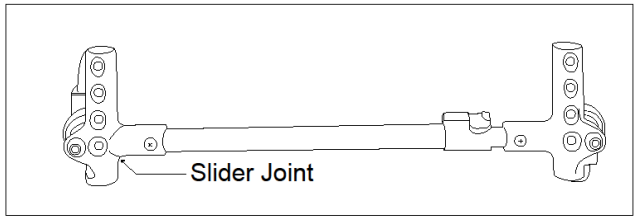

THE WRIGHT STUFF

Health Care Products that make life a little easier

Note:

- To maximize steering and performance, position the heavier wheelchair / occupant in the rear. Once you have decided on chair placement, set aside the lighter (Front) chair until the last step.
- The maximum wheel diameter that the Random Tandem can accommodate is 11”.

- Use the hex wrench provided to attach the two piece clamp collars to the left and right side of the wheelchair. They should be securely positioned near the front of the chair, approximately 8- 12” off the ground with the ball facing outward.
- Attach the Primary Section by loosening the snap collars and unfolding the extension arms. Pull back on the spring loaded quick release socket and release over the ball.
- Attach the wheeled section. Slide the plastic slider joint over the adjustment tubes and align with the appropriate spring button. The Wheeled section can be reversed (left to right) to accommodate a larger range of wheel sizes. The rear wheel of the front chair should be able to snugly drop between the cross bars.
- Adjust the pivot joint so that the adjustment tubes are level with the ground.
- Wrap the Velcro Wheel Sling around the front bar of the wheeled portion so that the wheel rests in it with approximately one inch clearance from the ground.
- Once you are satisfied with the arrangement, be sure to lock all Telescoping Slider Joints and you are ready to go!